)1 (Syringe size 5-6cc)
)2)Needle gage 22- 23)
)3 (Plunger color red)
)4 (Barrel color white)
)5 (Needle Tip color white)
)6 (Needle tip must be in one side of the syringe)
)7 (Rubber color black)

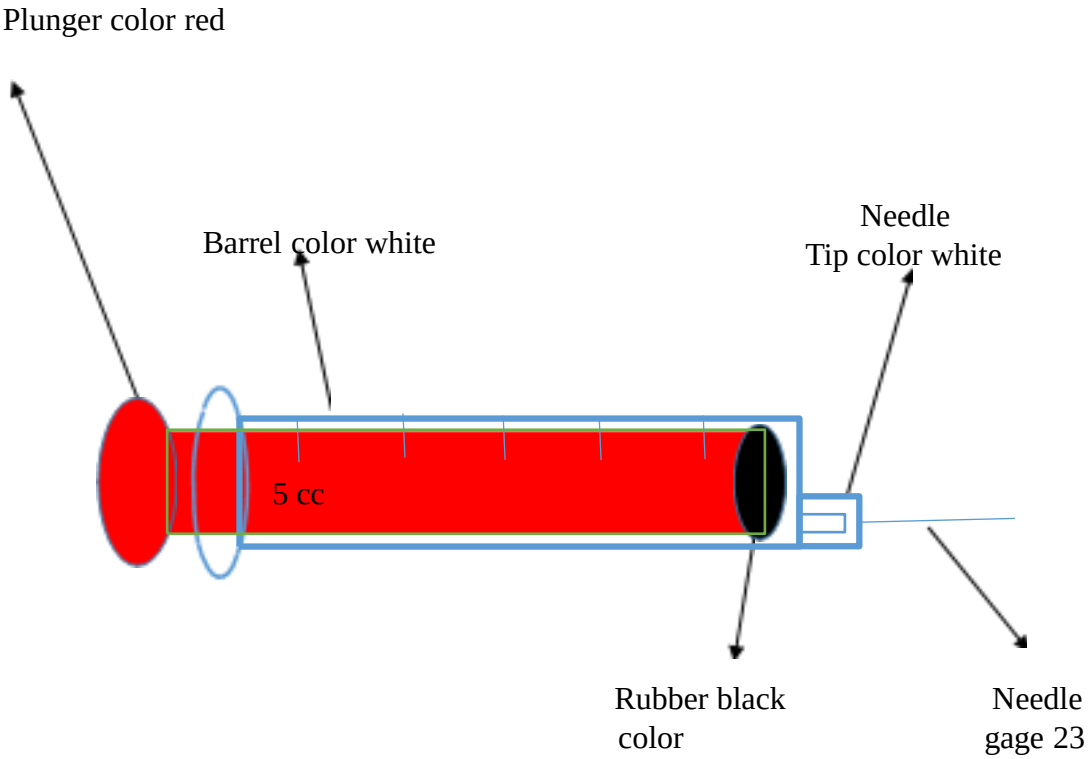

page one of plastic cover of the syringe to look like

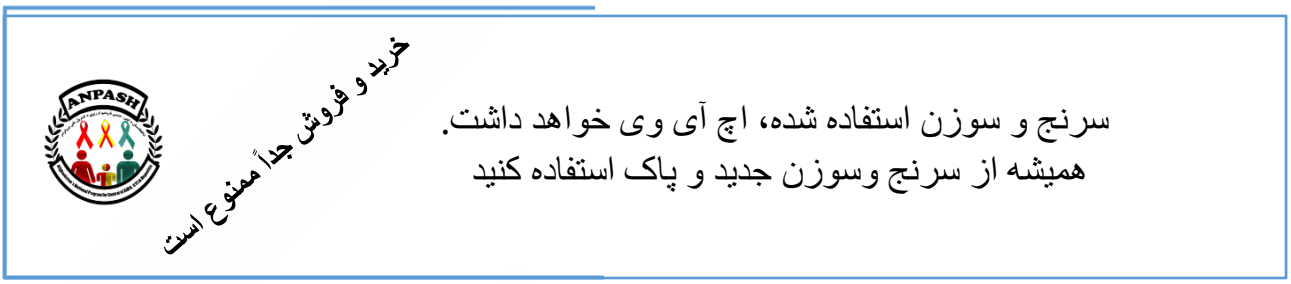

Page tow of the plastic cover of syringe to look like

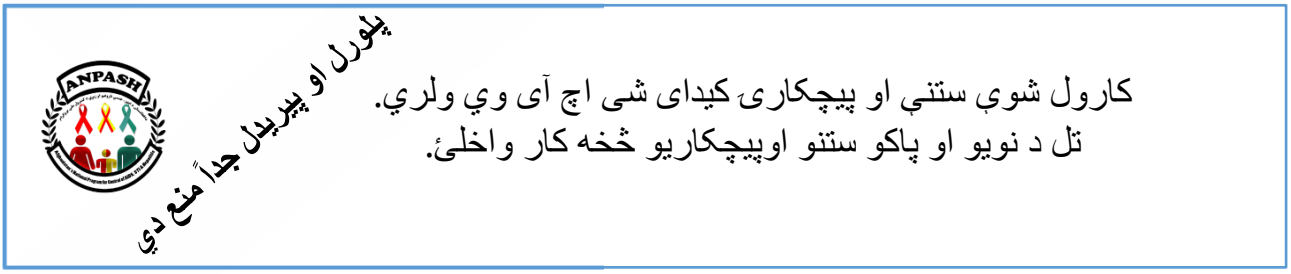

1) Translation of local language message ”Used needles and injections may contain HIV. Always use new and clean needles and syringes”.

For exact specification, please refer to RFP/ITB.

Figure 1: Mean Volume of Fluid Retained with Plunger Depressed

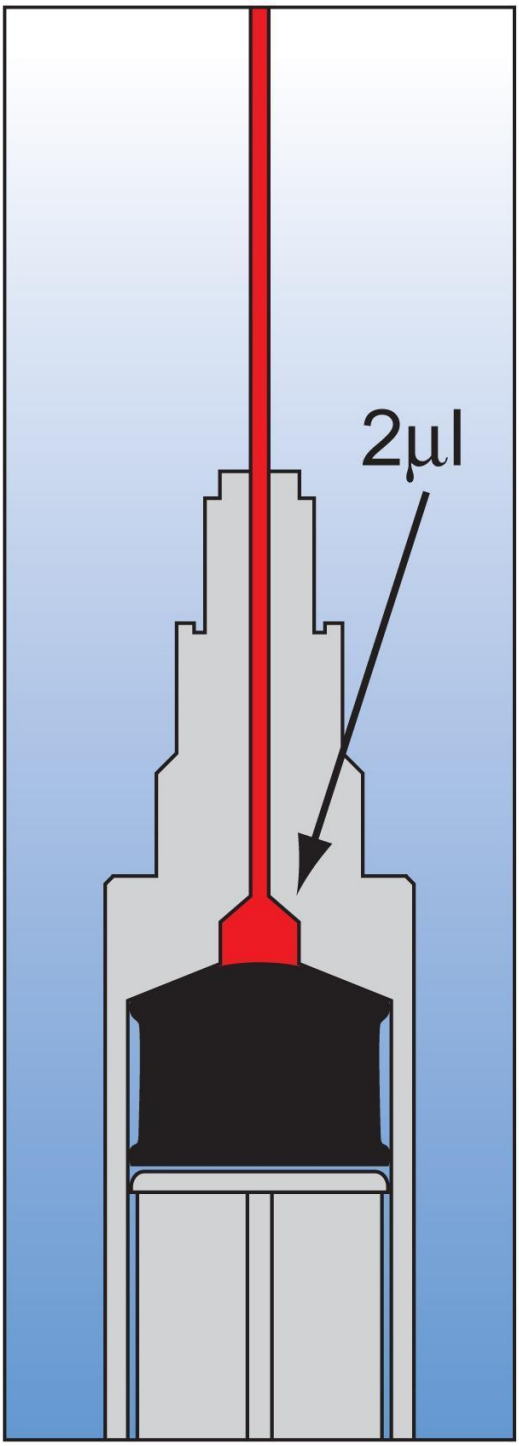

Low dead-space syringe

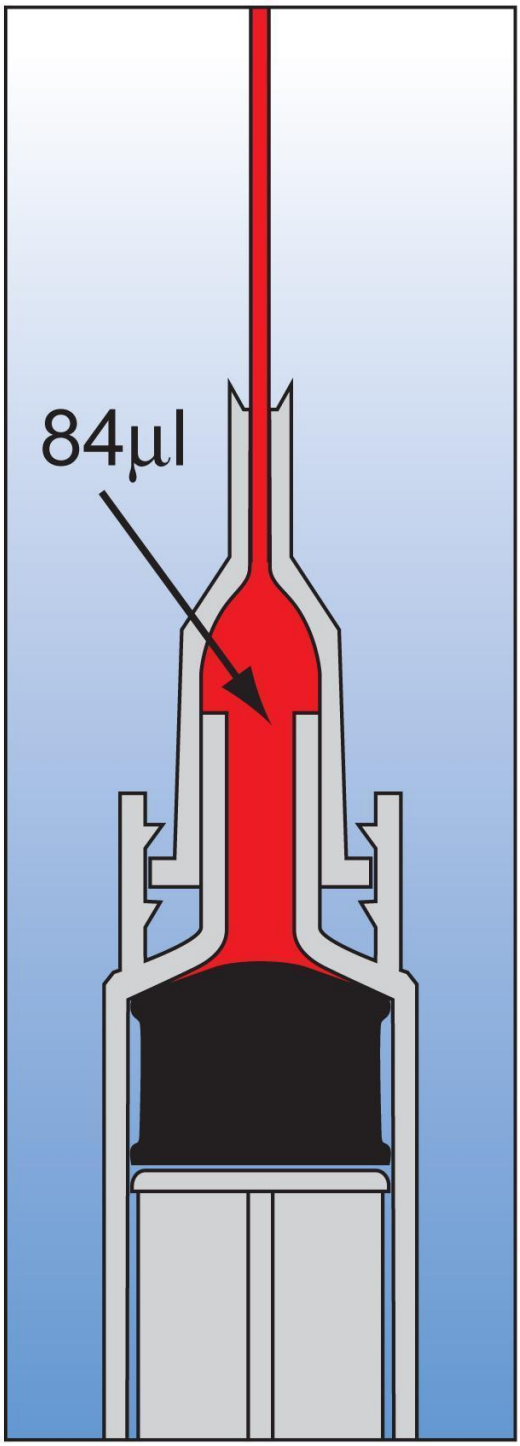

High dead-space syringe

The dead space must be very low, see attached pictures for comparison.

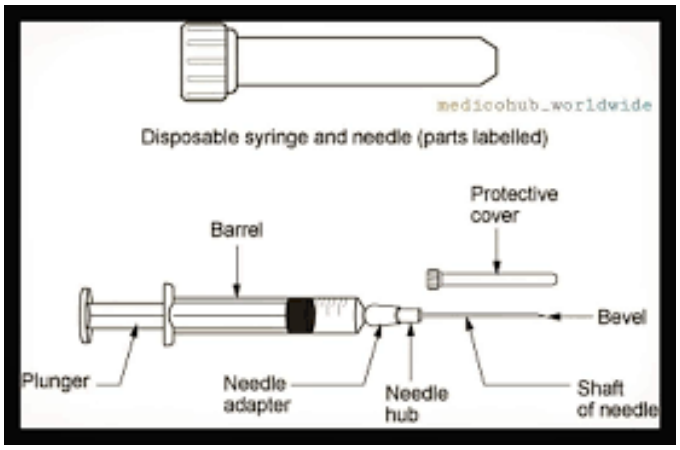

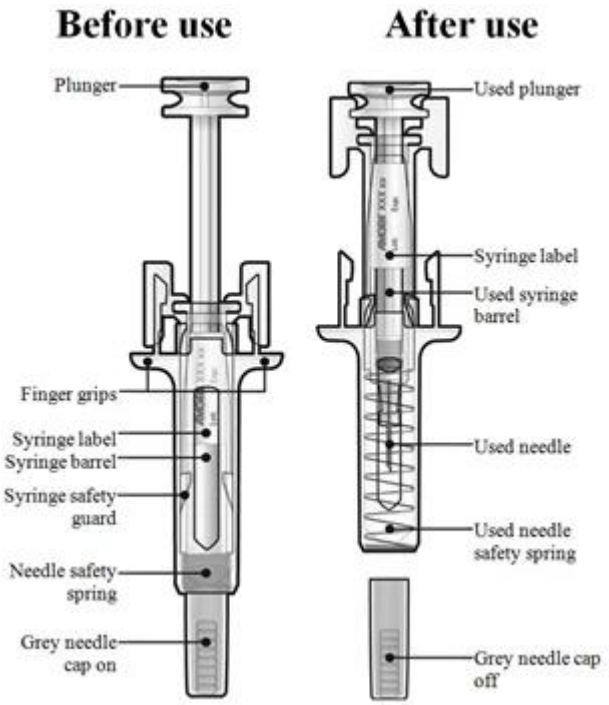

The needle to be tightened as screw into the syringe.